



100u 488, 561, 633 (3-5-3)

Cytometer:	FACSriaIII	User:	Administrator
Cytometer Name:	FACSriaIII	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 7.0
Input Device:	Manual	Date:	10/22/2014 4:40:07 PM
Sheath Pressure:	20.00		
Nozzle Size:	100		
Window Extension:	2.00		


Blue Laser
(488nm)
FSC

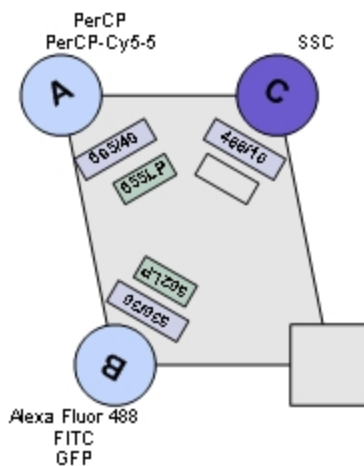

561 Yellow-Green Laser
(561nm)

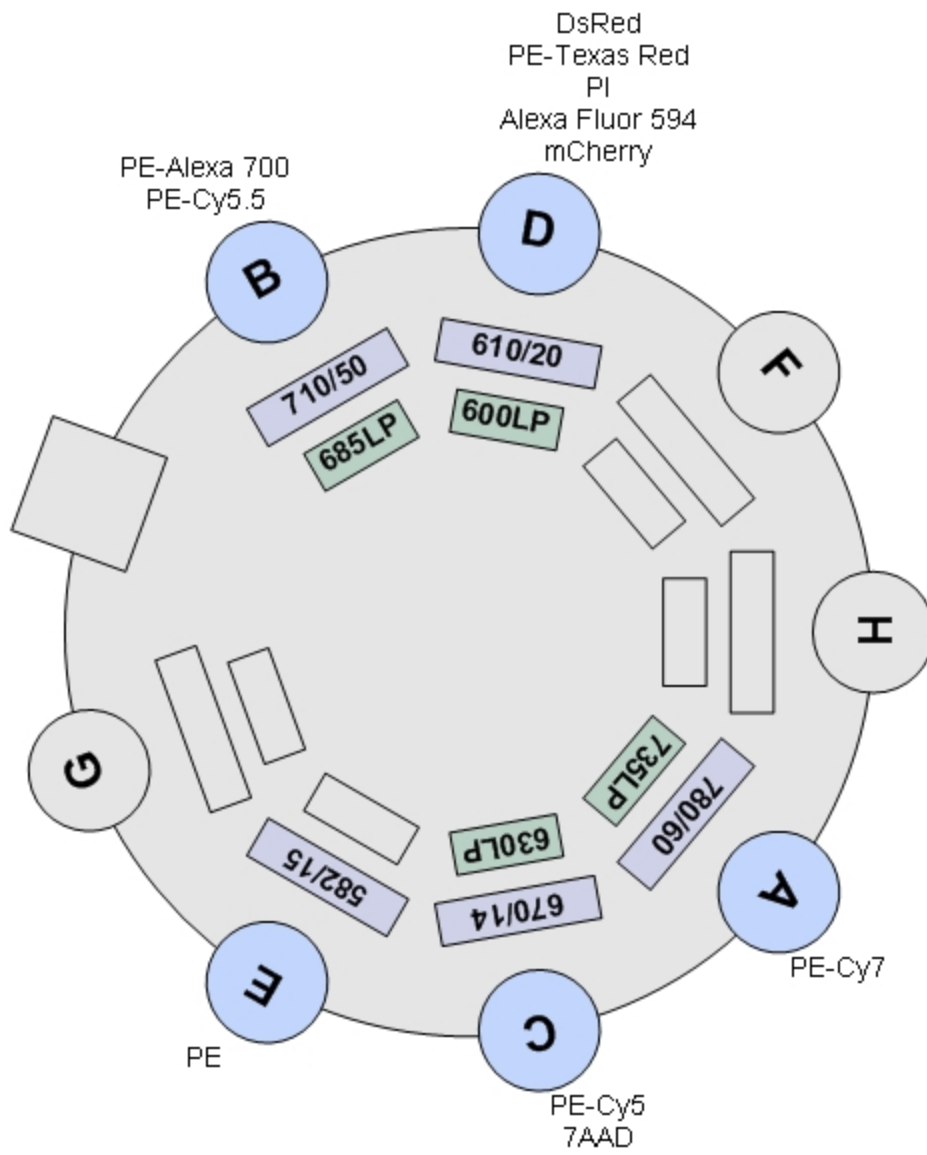

Red Laser
(633nm)

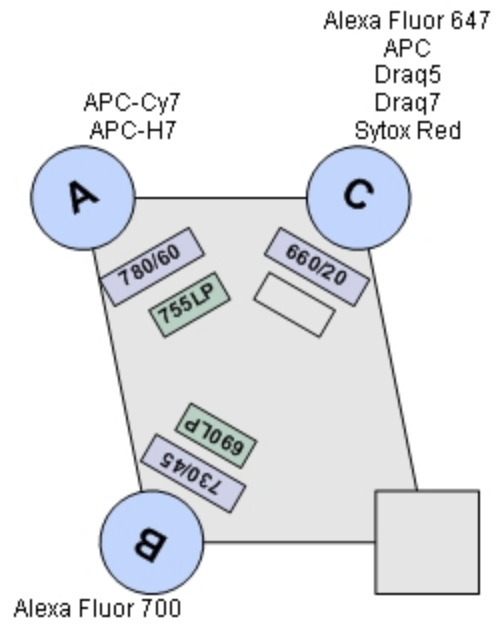

Comments:

1.5 density filter